003-2618-01
REV. B1

General Notes:
Outside edges of template indicate overall cabinet foot print. Position template in desired location per room layout drawing.

NOTE: HAVE A LICENSED PLUMBER AND ELECTRICIAN INSTALL ALL UTILITIES. LOCAL PLUMBING AND ELECTRICAL CODES SHOULD BE FOLLOWED FOR ALL CONNECTIONS. MIDMARK CORP. CANNOT BE HELD RESPONDSIBLE FOR INSTALLATIONS WHICH DO NOT CONFORM TO LOCAL CODES.

NOTE: To make installation easier and to prevent damage to area surrounding screw hole in floor, drill pilot holes. Use a 3/8 " masonry drill bit for concrete and a 9/32" wood drill bit for composite flooring.

TS4375/TS4385 ARTIZAN TREATMENT STATION
003-2618-01

TS4385

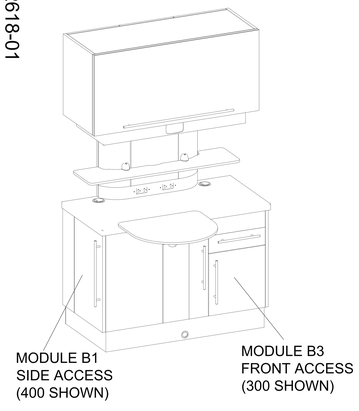

CONFIGURATION SHOWN

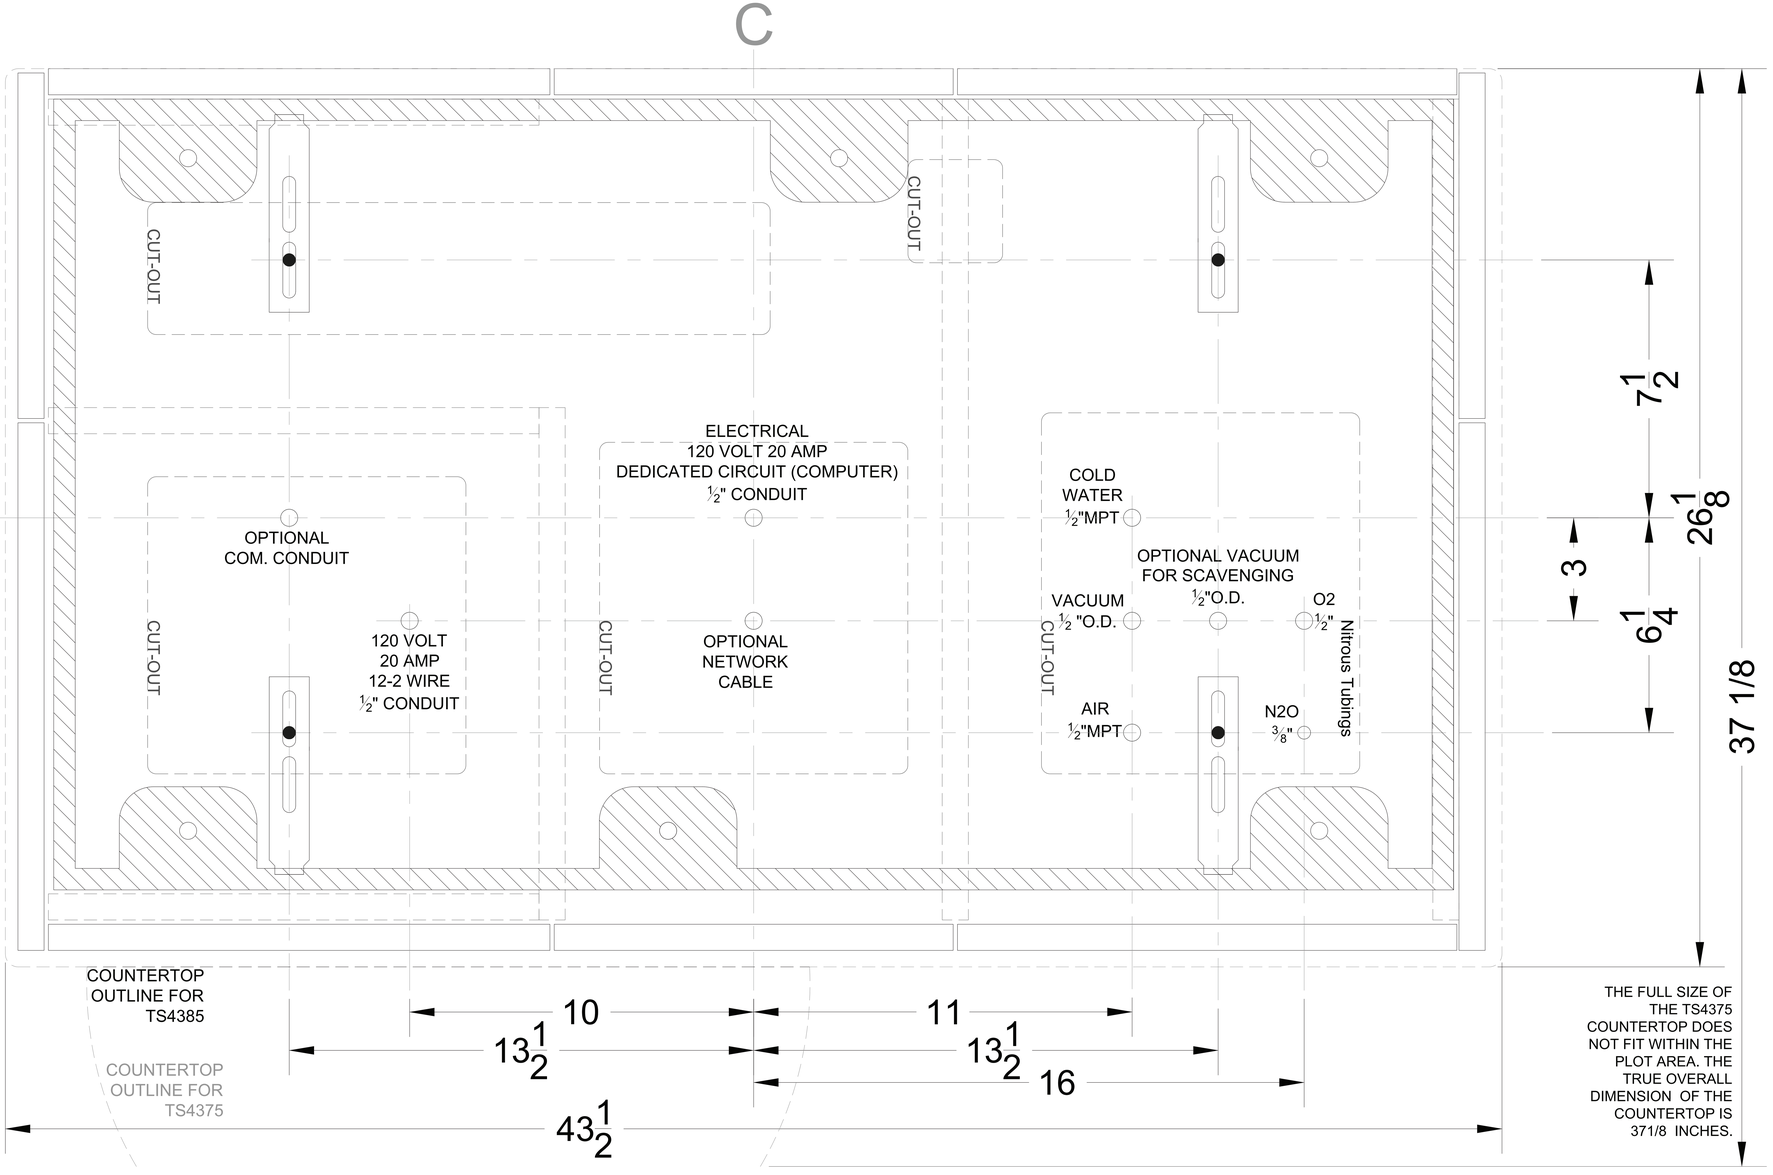

THE FULL SIZE OF THE TS4375 COUNTERTOP DOES NOT FIT WITHIN THE PLOT AREA. THE TRUE OVERALL DIMENSION OF THE COUNTERTOP IS 371/8 INCHES.

Electrical Specifications
1. Stub for electrical can be placed anywhere within the cut-out area. A recommended location has been indicated.
2. STANDARD: 3/4" diameter hole required for 1/2" NPT pipe stub. Stub to extend 1/2" from finished floor, under junction box (supplied by contractor). Wire per local electrical code.

Plumbing Secifications
1. Stubs for water, air , and vacuum can be placed anywhere within the cut-out area. Recommended locations have been indicated.
2. WATER: 3/4" diameter hole required for 1/2" NPT pipe stub. Stub to extend 2" min. / 2-1/2" max. from finished floor. Install manual shut-off valve (supplied with Midmark delivery unit).
Flush all debris from line before installing valve. Water pressure NOT to exceed 50 psi.
3. AIR: 3/4" diameter hole required for 1/2" NPT pipe stub. Stub to extend 2" min. / 2-1/2" max. from finished floor. Install manual shut-off valve (supplied with Midmark delivery unit).
Flush all debris from line before installing valve. Air pressure to be 80 psi (min.) to 100 psi (max.).
4. VACUUM: Plumbing to the casework should be specified by central vacuum supplier. Drill hole in floor as required. Extend pipe stub 2" min. / 2-1/2" max. from finished floor. Terminate plumbing with a 5/8" OD tubing connector.

TS4375/TS4385 ARTIZAN
TREATMENT STATION
SCALE: 1" = 1"
PLOT PAPER SIZE = 36" X 77"
NOTE: ALL PLUMBING PIPES SHOULD BE INSTALLED NO HIGHER THAN 5-1/4" ABOVE FINISHED FLOOR

MIDMARK

003-2618-01
TS4375/TS4385 ARTIZAN TREATMENT STATION