



EASE
EQUIPMENT ANCHORAGE & SEISMIC ENGINEERING
2801 Connery Way Suite B
Missoula, MT 59808
Phn: (406) 541-3273 Fax: (406) 541-3274

Office of Statewide Health Planning and Development
ANCHORAGE PRE-APPROVAL

OPA-2376-07

Equipment Manufacturer: Midmark

Equipment Type: Instrument Panel

GENERAL NOTES

1. FORCES PER ASCE 7-05 SECTION 13.3.1, EQUATIONS 13.3-1, 13.3-2 & 13.3-3, WHERE $S_{DS} = 1.93$, $a_p = 1.0$, $I_p = 1.5$ & $R_p = 2.5$
2. THIS PRE-APPROVAL CONFORMS TO THE 2007 CALIFORNIA BUILDING CODE.
3. THE DETAILS IN THIS PRE-APPROVAL MAY BE USED AT ANY HEIGHT AND AT ANY LOCATION IN THE STATE OF CALIFORNIA.
4. ALL ANCHOR FORCES SHOWN ON THE DRAWINGS ARE WORKING LOADS (AS OPPOSED TO STRENGTH LEVEL LOADS) AND MAY BE USED FOR ALLOWABLE STRESS DESIGN.
5. SHEET METAL SCREWS SHALL BE TEKS SCREWS BY ITW BUILDEX (ICC ESR-1976).
6. PER CAN 2-1708A.5, THIS UNIT DOES NOT REQUIRE "SPECIAL SEISMIC CERTIFICATION".

RESPONSIBILITIES OF THE STRUCTURAL ENGINEER OF RECORD


7. DESIGN BACKING BARS, STUDS, ETC. WHICH THE UNITS ARE ATTACHED TO AS NOTED ON THE DRAWINGS. THE SEOR SHALL ALSO VERIFY THE ADEQUACY OF THE STRUCTURES (SUCH AS WALLS AND FLOORS) WHICH SUPPORT THE UNITS FOR THE LOADS IMPOSED ON THEM BY THE UNITS AS WELL AS ALL OTHER LOADS.
8. PROVIDE ANY SUPPORTING STRUCTURE REQUIRED TO SUPPORT WEIGHTS AND FORCES SHOWN, IN ADDITION TO ALL OTHER LOADS.
9. VERIFY THAT THE INSTALLATION IS IN CONFORMANCE WITH THE 2007 CBC AND WITH THE DETAILS SHOWN IN THIS PRE-APPROVAL. VERIFY THAT THE ACTUAL EQUIPMENT'S WEIGHT, CG LOCATION, ANCHOR LOCATIONS, ANCHOR DETAILS AND THE MATERIAL AND GAGE OF THE UNIT WHERE ATTACHMENTS ARE MADE AGREE WITH THE INFORMATION SHOWN ON THE PRE-APPROVAL DOCUMENTS.



MIDMARK INSTRUMENT PANEL	DES. R. LA BRIE	SHEET 2 OF 3 SHEETS
	JOB NO. 11-0989	
	DATE 9/28/09	

SEISMIC ANCHORAGE

WALL MOUNTED

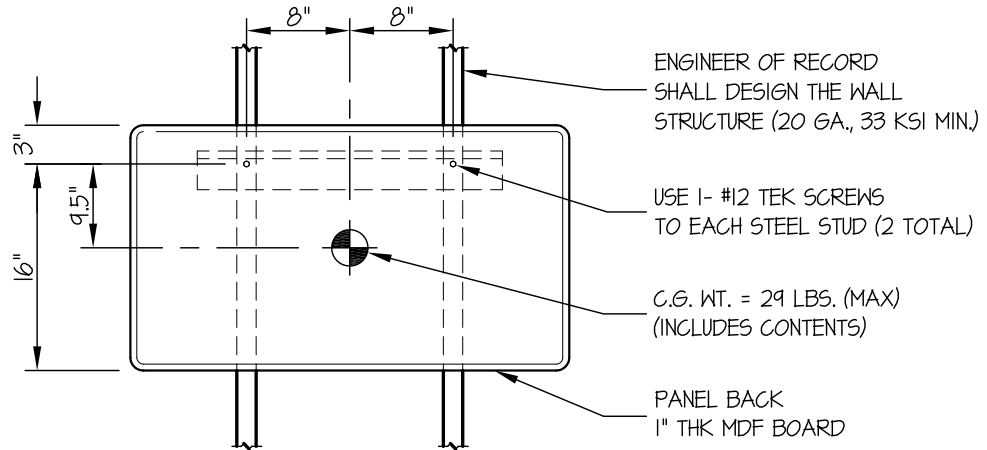

FRONT ELEVATION

NOTES:

1. ANCHORAGE DESIGN PER 2007 CALIFORNIA BUILDING CODE - SECTION 1613A AND ASCE 7-05 SECTIONS 12 AND 13. ALLOWABLE STRESS DESIGN IS USED.

HORIZONTAL FORCE (E_H) = $0.97 W_p$ ($S_{DS} = 1.93, a_p = 1.0, I_p = 1.5, R_p = 2.5$)


VERTICAL FORCE (E_v) = $0.27 W_p$

$T_{MAX} = 59$ LBS/SCREW
 $V_{MAX} = 33$ LBS/SCREW

2. CENTER OF GRAVITY (C.G.) WEIGHT IS A MAXIMUM. THIS PRE-APPROVAL ENCOMPASSES ALL WEIGHTS UP TO THE MAXIMUM WEIGHT SHOWN.

3. ENGINEER OF RECORD FOR THE BUILDING SHALL PROVIDE SUPPORT STRUCTURE DESIGNED TO SUPPORT WEIGHTS AND FORCES SHOWN, IN ADDITION TO ALL OTHER LOADS.

4. SEE GENERAL NOTES: SHEET 1.

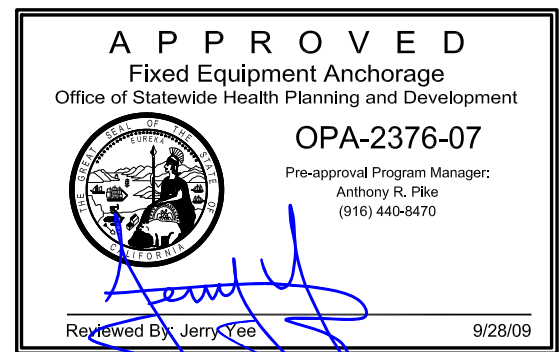

<h1>MIDMARK</h1> <h2>INSTRUMENT PANEL</h2>	DES. R. LA BRIE	SHEET 3
	JOB NO. 11-0989	OF 3 SHEETS
	DATE 9/28/09	

SEISMIC ANCHORAGE

WALL MOUNTED


5/8" THK. WALL BOARD

ENGINEER OF RECORD SHALL DESIGN THE WALL STRUCTURE (20 GA., 33 KSI MIN.)

C.G. WT. = 29 LBS. (MAX)
(INCLUDES CONTENTS)

USE 1- #12 TEK SCREWS TO EACH STEEL STUD (2 TOTAL)

PANEL BACK
1" THK MDF BOARD

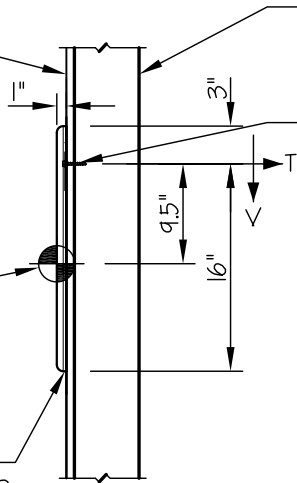

SIDE ELEVATION AT STEEL STUD WALL

2 x STUDS OR 4 x BLKG (DOUGLAS-FIR LARCH NUMBER 2 MIN.) (DESIGNED BY ENGINEER OF RECORD)

USE 1- 1/4" ϕ X 3" LAG BOLTS AT EACH WOOD STUD OR BLKG. (PRE-DRILL HOLES TO SHANK DIAMETER)

5/8" THK. WALL BOARD



SIDE ELEVATION AT WOOD STUD WALL

