



**Support on Demand (User Reference Guide)**  
**937-526-8445 or 1-800-Midmark, ext. 8445**

**24 Hour Technical Support**

Midmark's Support on Demand is an automated service that gives you 24/7 access to technical information. This easy to use service offers everything from sterilizer operating instructions to anesthesia machine leak test instructions. The parts identification portion of this service includes approximately ten of the most requested part numbers.

With Support on Demand, you can use the easy-to-follow instructions to navigate, or use the reference codes listed on this guide.

When using Support on Demand, you may press the 'pound' key to return to the previous menu, or you may press the 'star' key to return to the main menu, re-enter the reference code and replay an instruction.

Note: Dialing 937-526-8445 will connect you directly to the 24 hour technical support menu.

Quick Tips: Dial 937-526-8445 and make a selection from the 24 hour technical support menu. When the Support on Demand main menu is played, enter a reference code listed on this guide to quickly get the instruction needed.

Example: If you would like VME2™ leak test instructions, dial 937-526-8445 and select Support on Demand for anesthesia products. When you hear the Support on Demand main menu, enter reference code 132 and your instruction will automatically play.

<b>Sterilizers</b>	<i>Reference Code</i>
<b><u>M3 Ultrafast®</u></b>	
Installation Instructions .....	411
Accessory Information .....	412
Operating Instructions .....	4211
Standard Cycle Parameters .....	4212
Frequently Asked Questions.....	423
Error Codes .....	424
Periodic Maintenance .....	4221
Monthly Maintenance .....	4222
Priming Instructions.....	4223
<b><u>Current Generation M9/M11 Sterilizer (w/ Green Display)</u></b>	
Operating Instructions .....	1111
Standard Cycle Parameters .....	1112
Weekly Maintenance .....	1121
Monthly Maintenance .....	1122
Frequently Asked Questions.....	113
Error Codes .....	114
<b><u>First Generation M9/M11 Sterilizer (w/ Red Display)</u></b>	
This product has reached its end of life.	
Midmark no longer provides service parts or support for this product.	
<b><u>M7 Speedclave® (Models 020-022)</u></b>	
Operating Instructions .....	3111
Time & Temperatures .....	3112
Weekly Maintenance .....	3121
Monthly Maintenance .....	3122
Frequently Asked Questions.....	313
<b><u>1st &amp; 2nd Generation M7 (Models 001-016)</u></b>	
These products have reached their end of life. Midmark no longer provides service parts or support for these products.	

<b>Matrx™ Anesthesia Machines</b>	<i>Reference Code</i>
Frequently Asked Questions.....	14
Accessory Information .....	112
<b><u>VMC® Anesthesia Machine</u></b>	
VMC® Leak Test Instructions .....	131
VMC® Flow Meter Repair Information.....	1521
VMC® Absorber Assembly Parts List .....	1522
VMC® Anesthesia Machine Parts List.....	1523
VMC® Maintenance Schedule .....	1211
VMC® Maintenance Kit Instructions.....	1212
VMC® Stand Mount Installation Instructions .....	1113
<b><u>VME2™ Anesthesia Machine</u></b>	
VME2™ Leak Test Instructions .....	132
VME2™ Flow Meter Parts List.....	1531
VME2™ Anesthesia Machine Parts List .....	1532
VME2™ Maintenance Schedule .....	1221
VME2™ Maintenance Kit Instructions .....	1222
VME2™ Installation Instructions .....	1114
<b><u>VMS® &amp; VMS® Plus Anesthesia Machine</u></b>	
VMS® & VMS® Plus Leak Test Instructions.....	131
VMS® & VMS® Plus Flow Meter Parts List.....	1511
VMS® & VMS® Plus Absorber Assembly Parts List.....	1512
VMS® & VMS® Plus Anesthesia Machine Parts List .....	1513
VMS® & VMS® Plus Maintenance Schedule .....	1211
VMS® & VMS® Plus Maintenance Kit Instructions .....	1212
VMS® Wall Mount Installation Instructions.....	1112
VMS® & VMS® Plus Stand Mount Installation Instructions ..	1111



<b>Matrx™ Tech Three Vaporizers</b>	
Service Information.....	22
Frequently Asked Questions.....	23
VMS®, VMS® Plus & VME2™ Installation Instructions .....	211
VMC® Installation Instructions .....	212

<b>Matrx™ Ventilator Products</b>	
Accessory Information .....	31
Service & Parts Information.....	32

**Note: Always follow safety instructions listed in your manual.**

Visual Reference on Back

## Tubing Diagrams

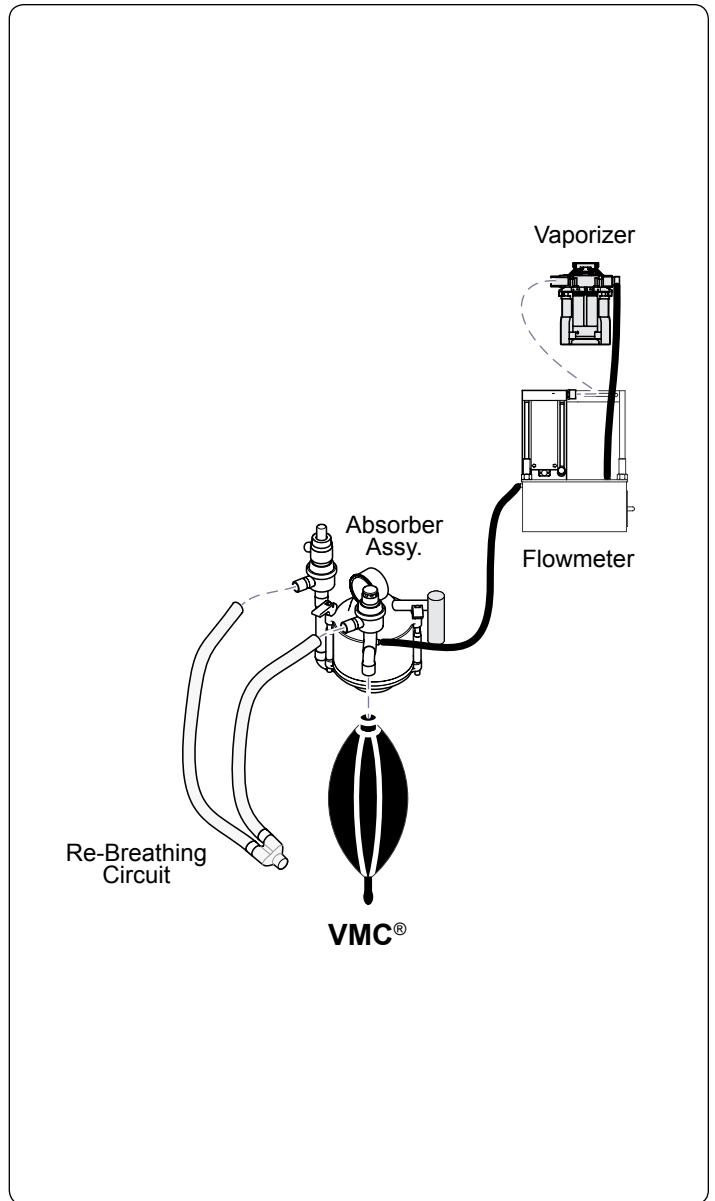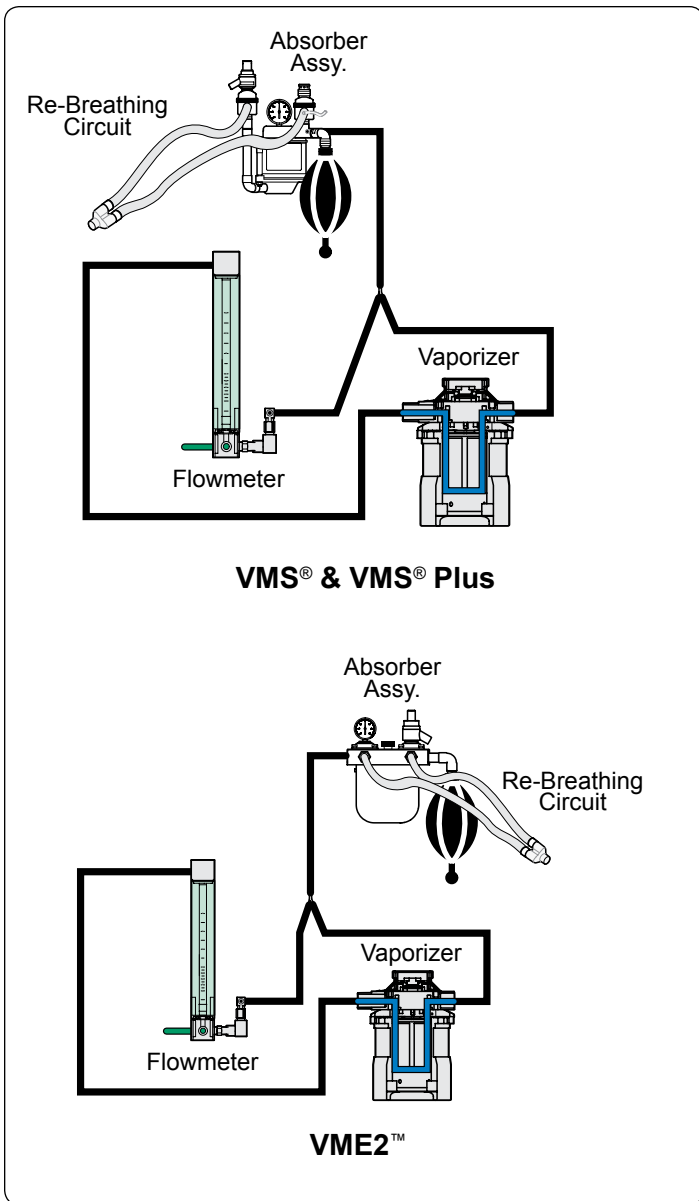

## Leak Test

