midmark®

MEDICAL

626 Barrier-Free® Examination Chair



Better care begins with better design

Did you know that nearly half of the adult population in the US has hypertension?[1] That leaves them at higher risk for heart disease. We know how important it is for you to help your patients live their healthiest, happiest lives. That's why capturing an accurate blood pressure (BP) measurement is so important—better BP is better care.



Improving Patient Health Better BP®

Standardization can be tough. Many healthcare providers have reported not following American Heart Association (AHA) recommendations for more accurate BP measurement.[2]

ONE OF THE BIGGEST AREAS FOR OPPORTUNITY

- Nearly **1 of every 2** US adults have high BP.[1]
- **12.4%** increase in U.S. adults classified as having high blood pressure when measured BP was modeled 5 mmHg higher systolic and 3.5 mmHg higher diastolic.[3]
- **23.6 million** Additional U.S. adults estimated to have high blood pressure when measured BP was modeled 5 mmHg higher systolic and 3.5 mmHg higher diastolic.[4]

COSTS RELATED TO IMPROPER BP MEASUREMENT + HYPERTENSION MISDIAGNOSIS

1,933
Typical number of patients for one physician[5]

$197,000
Average annual cost of hypertension per practicing physician[6]

$521
Annual cost of hypertension per patient[6]

ACCURATE PATIENT POSITIONING + SEAMLESS CONNECTIVITY

Midmark designed the first and only fully integrated point of care ecosystem that has been clinically validated to achieve improved accuracy for a resting BP. Connectivity at the point of care allows patient data to be transferred directly into the EMR, reducing manual entry and further improving the vital signs workflow.

1. LOW HEIGHT
The 15.5" low seat height helps patients keep their back supported and feet flat on the floor.

2. PROPER ARM PLACEMENT
The articulating arm rail supports the patient's arm with cuff at heart height.

3. VITAL SIGNS
An automated, connected vital signs device promotes consistency and data accuracy.


4. CONNECTED DEVICES
EMR connectivity improves workflow efficiency and helps reduce the likelihood of errors.

5. WORKFLOW EFFICIENCY
Connect the Midmark vital signs device to the 626 exam chair with integrated digital scale to weigh patients quickly and discreetly from the exam chair, then transfer data to the patient record.

6. UNIFIED INTERFACE
Midmark Connect provides a seamless connection between your devices and the EMR. Operate all of your devices from one single pane of glass—the computer screen.



What happens today?

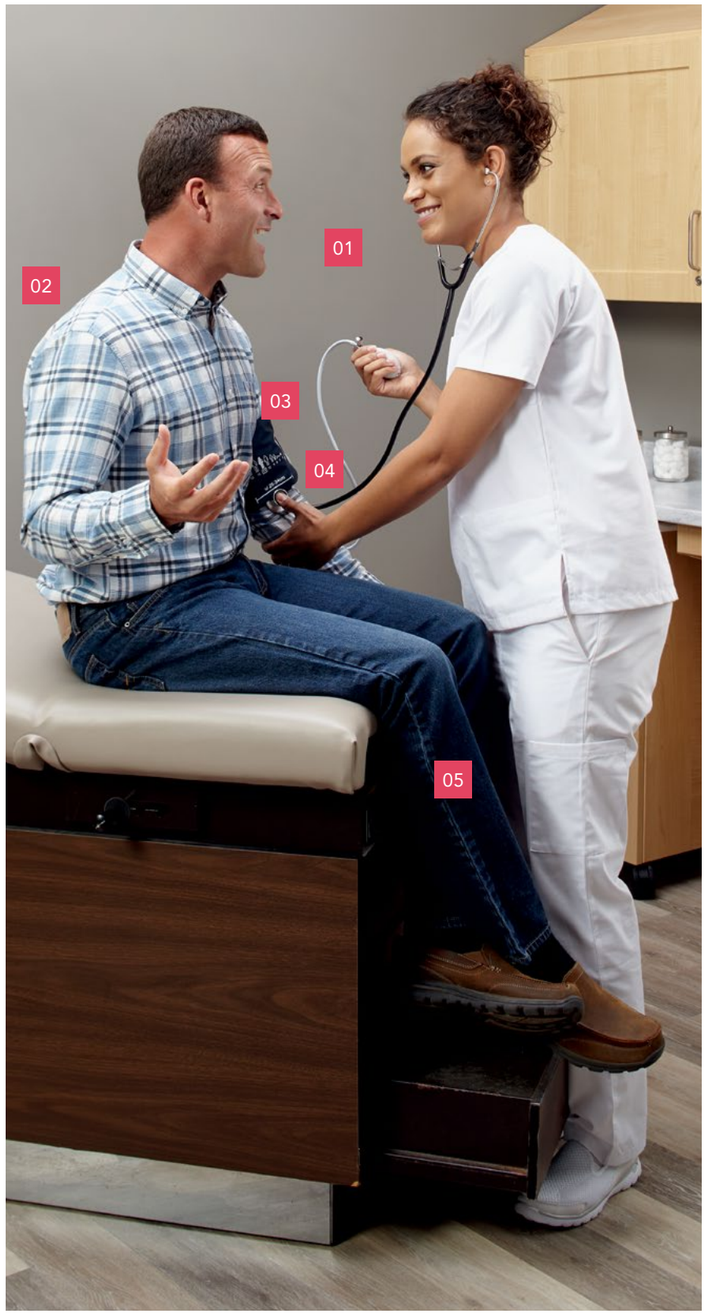

Taking BP with a patient seated on an exam table rather than in an AHA-recommended position resulted in readings averaging 7.0 mmHg higher systolic and 4.5 mmHg higher diastolic.[7] Reviews suggest that even a difference of 5 mmHg can affect close to 12.4% of patients, either inadvertently placing them on medication or missing a diagnosis of hypertension.[3]

01 Talking


02 Back not supported

03 Cuff placed over clothing

04 Arm not supported with cuff at heart level

05 Legs crossed and feet not flat on floor

There's a better way.

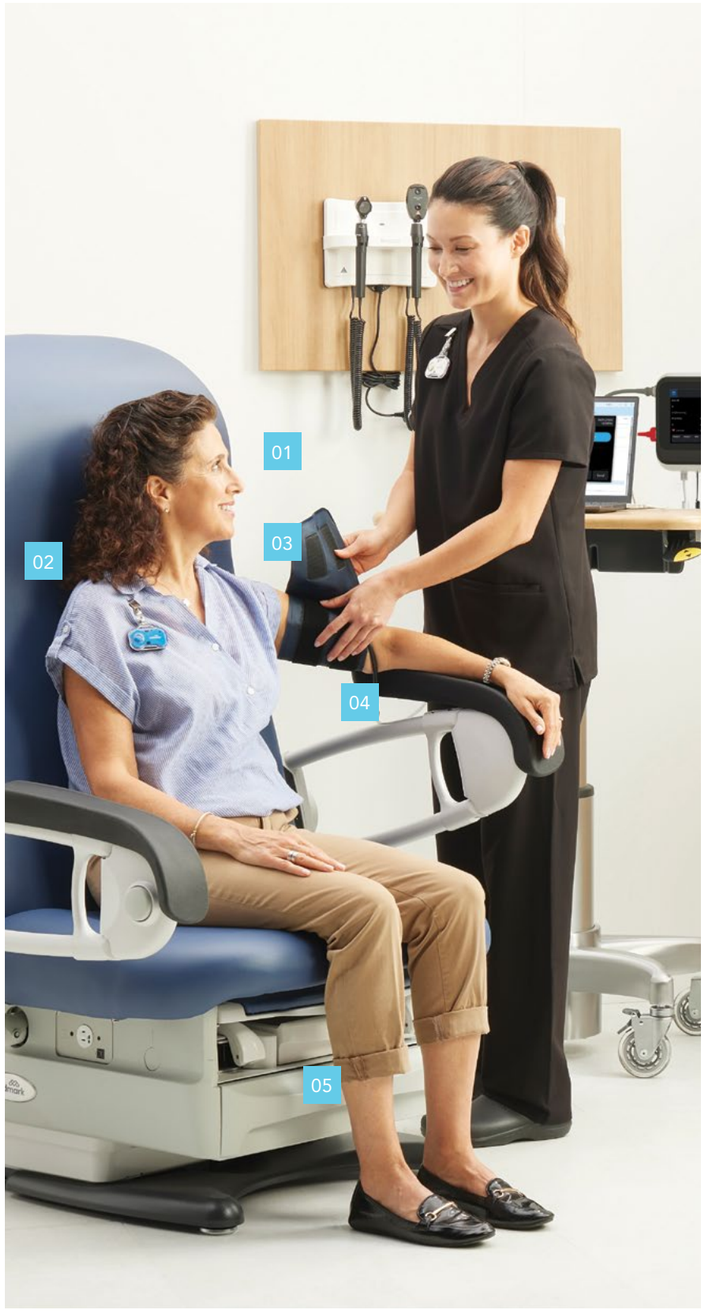

The good news is new technologies and equipment have been designed to help clinicians follow clinical standards for blood pressure capture. Midmark has developed a suite of products that are designed to function as a fully integrated, point of care ecosystem to help health systems standardize and promote proper blood pressure capture through improved patient positioning.[8]

01 Not talking

02 Back supported

03 Cuff placed on bare arm

04 Arm supported with cuff at heart height

05 Legs uncrossed and feet flat on floor

Accessible Design
Equal Care for All







Midmark 626
Barrier-Free®
Examination Chair

Help patients help themselves

The Midmark 626 Barrier-Free® Examination Chair is an ideal solution for accessible patient care. Compliant with the 2024 US Access Board Standards for Accessible Medical Diagnostic Equipment,[9] the Midmark 626 features a low seat height of 15.5 inches, making it easier for patients with mobility challenges to transfer independently. **This chair not only meets but exceeds the Access Board requirement for a maximum low seat height of 17 inches, distinguishing itself as the only chair currently on the market to achieve this level of accessibility.**

In addition to its low height, the Midmark 626 provides an adjustable transfer surface, ensuring that caregivers can raise the chair to an ergonomic height, reducing the risk of injury. There is also the option of adding support rails and knee crutches for compliance and patient stability, further enhancing safety during transfers and examinations. For clinics looking to improve both patient access and caregiver safety, this chair represents a crucial advancement.

SCAN TO LEARN MORE.

SCAN TO SEE A PATIENT TRANSFER.









Features

Models + Options

	14.6" Seat Height (Compressed) 15.5" Seat Height (Uncompressed)	Clean Assist Roller System	Active Sensing Technology	Lockout Hand + Foot Controls	Wireless Hand + Foot Controls	Wired Hand + Foot Controls	Heated Upholstery	Digital Scale	650 lb Weight Capacity	Standard Rail Accessory Receivers	Tamper-Resistant Electrical Receptacles	Drawer Heater + Pelvic Tilt
Midmark												
626-001	•	•	•	•		•			•	•	•	•
626-002	•	•	•	•		•	•		•	•	•	•
626-003	•	•	•	•	•			•	•	•	•	•
626-004	•	•	•	•	•		•	•	•	•	•	•
626-005	•	•	•	•		•		•	•	•	•	•
626-006	•	•	•	•		•	•	•	•	•	•	•

Optional Features

(Available on select models)



DIGITAL SCALE

Capture the patient's weight discreetly from the comfort and security of the exam chair with the integrated digital scale, and transfer data directly into the EMR when paired with a vital signs device.



HEATED UPHOLSTERY

The heated upholstery option provides soothing heat to help relax the patient while on the exam chair.

STANDARD FEATURES



CLEAN ASSIST ROLLER SYSTEM

The retractable roller base allows you to safely move the chair for cleaning.



HAND + FOOT CONTROL

Hand/foot control designed to make patient positioning quick and effective.



STIRRUPS + PELVIC TILT

Help position patients properly and comfortably for lower body examinations.



ACTIVE SENSING TECHNOLOGY®

Pauses chair movement when disrupting impact is detected.



QUICK EXAM® + RETURN TO HOME

Quick Exam elevates the chair to the exam position. Return to Home returns the chair to its home position.



ACCESSORY RECEIVERS

Standard receivers allow for the integration of accessories without the use of tools.



TAMPER-RESISTANT RECEPTACLES

Receptacles on both sides of the chair provide a power connection for devices.



PREMIUM COMFORT SYSTEM®

Elastomeric material stretched over a seat cutout for a chair-like feel.



DRAWER HEATER

Point of care storage with the option to warm supplies used for lower body examinations.



LOCKOUT OF HAND + FOOT CONTROLS

Prevent unintended movement of the chair when staff is away by using the lockout controls (located on either the hand or foot control) to lockout controls on both the hand and foot control.




Accessories

Accessories help add versatility + function to your exam chair

ACCESSORIES



PATIENT SUPPORT RAILS+
Required for US Access Board Compliance.
Help achieve proper positioning of the patient's arm for blood pressure capture and phlebotomy procedures.

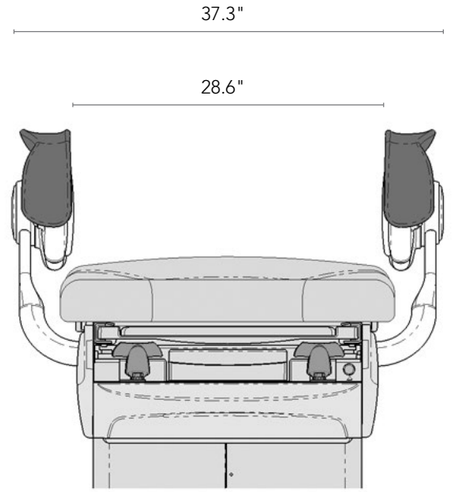

Patient Support Rails+ Dimensions



PATIENT SUPPORT RAILS
Required for US Access Board Compliance. Provide patients with a 1.25" inch diameter continuous gripping surface for entering, exiting or repositioning on the exam chair.



WIRELESS CONTROLS
Locate the hand and foot control anywhere in the room, removing cords and eliminating obstacles.



ARTICULATING KNEE CRUTCHES
Required for US Access Board Compliance. Enhance patient leg support and comfort during lower body exams.



RITTER® 253 LED LIGHT
The 253 is designed with easy access controls, high intensity light and an adjustable focal spot. Available in chair mount and mobile options.



STAINLESS STEEL TREATMENT PAN
Ideal for lower body procedures or other situations in which removal of fluid and debris is necessary.

COLOR OPTIONS

STANDARD UPHOLSTERY COLORS

- Mist 813
- Stone 814
- Restful Path 858
- Iron Ore 851
- Lunar Gray 845
- Obsidian 857
- Oasis 843
- Soothing Blue 855
- Dream 847
- Mineral 844
- Healing Waters 848
- Shaded Garden 853
- Citrus 849
- Sandy Retreat 850
- Curative Copper 846
- Cranberry 859
- Dark Linen 856
- Latte 860
- Robust Brown 852
- Deep Earth 854

ULTRAFREE UPHOLSTERY COLORS

- UltraFree Stone 865
- UltraFree Restful Path 868
- UltraFree Obsidian 867
- UltraFree Harbor 861
- UltraFree Wheatgrass 862
- UltraFree Spice 863
- UltraFree Cranberry 869
- UltraFree Dark Linen 866
- UltraFree Latte 870
- UltraFree Branch 864

SERVICES + SUPPORT

TECHNICAL SPECIFICATIONS
View technical specifications for the Midmark 626 Barrier-Free® Examination Chair.

SCAN TO VIEW SPECS.

MIDMARK LIVE DESIGN
Our in-house design experts are ready to help you every step of the way.

SCAN TO VIEW VIDEO.

MIDMARK DELIVERY SERVICES
Coordination, delivery and setup right on time, every time.

SCAN TO VIEW YOUR OPTIONS.

CLINICAL EDUCATION
Trust in our expert educators to assist in implementing your Midmark devices.

SCAN FOR TRAINING OPTIONS.

REPAIR + SERVICE
Explore available support and service plans so you can obtain the level of coverage you need to keep your medical equipment and devices operational. This includes periodic maintenance and periodic inspection plans, as well as extended warranty plans.

SCAN FOR SUPPORT.

CONTACT US
Curious about our products and services or have a general inquiry? We're here to help. Tell us how to contact you and we'll be in touch with more details.

SCAN TO VIEW.

SOURCES

01 https://newsroom.heart.org/news/new-high-blood-pressure-guideline-emphasizes-prevention-early-treatment-to-reduce-cvd-risk

02 https://newsroom.heart.org/news/some-health-care-professionals-use-outdated-guidelines-to-screen-and-diagnose-hypertension

03 Sakhuja, S., Jaeger, B.C., Akinyelure, O.P., (...), Muntner, P. (2022) Potential impact of systematic and random errors in blood pressure measurement on the prevalence of high office blood pressure in the United States. Journal of Clinical Hypertension. https://doi.org/10.1111/jch.14418

04 Sakhuja, S., Jaeger, B.C., Akinyelure, O.P., (...), Muntner, P. (2022) Potential impact of systematic and random errors in blood pressure measurement on the prevalence of high office blood pressure in the United States. Journal of Clinical Hypertension. https://doi.org/10.1111/jch.14418

05 https://pmc.ncbi.nlm.nih.gov/articles/PMC12978577

06 https://pmc.ncbi.nlm.nih.gov/articles/PMC11425759/

07 Alpert BS, Schwartz JE, Shapiro M, Wexler RK. Comparison of outcomes for routine versus American Heart Association-recommended technique for blood pressure measurement (CORRECT BP): a randomised cohort study. EClinicalMedicine. 2023 Sep 14;64:102219. doi: 10.1016/j.eclinm.2023.102219. PMID: 37745022; PMCID: PMC10515304.

08 https://www.ahajournals.org/doi/10.1161/HYP.0000000000000249?utm_campaign=sciencenews25-26&utm_source=science-news&utm_medium=phd-link&utm_content=phd-08-14-25

09 https://www.federalregister.gov/documents/2024/07/25/2024-16266/standards-for-accessible-medical-diagnostic-equipment



Designing better care.®

USGBC
MEMBER

CARB 93120.2 Phase 2 Compliant and TSCA Title VI Compliant

The color examples shown are the best representation of the original material. Actual color may vary slightly. We strongly recommend that you contact Midmark Customer Experience at 1.800.MIDMARK to request a sample before placing your order.

USGBC® and the related logo are trademarks owned by the U.S. Green Building Council® and are used with permission.

Midmark is an ISO 13485 and ISO 9001 Certified Company. Certain products are not included. See the complete list at: midmark.com/ISO

For more information, contact your authorized Midmark distributor or call: 1.800.MIDMARK
Outside the USA call: 1.937.526.3662 or visit our website: midmark.com

© 2026 Midmark Corporation, Versailles, Ohio USA
Products subject to improvement changes without notice.

007-10267-00 Rev. D1 (10/26)

midmark®