



MEDICAL

631 Procedure Chair

 midmark

Elevating Care for all Patients



As patient needs evolve and in-office procedures continue to increase, Midmark is dedicated to designing environments that elevate the standard of care. Are you ready to support the future of patient-centered, accessible healthcare?




Preparing for the Future of Patient Care—Starting Today

Healthcare is changing—more patients, more in-office procedures and a growing demand for accessibility. Obesity, the aging population and disabilities are on the rise creating new challenges for healthcare providers every day. You may feel that your current equipment is adequate but there could be opportunities to better meet the needs of your patients. **In fact, 73% of US adults feel the healthcare system is failing to meet their needs in at least one way.**¹

ARE YOUR PROCEDURE CHAIRS COMPLIANT?


In 2024, the US Access Board (USAB) issued a new standard² establishing design criteria for medical diagnostic equipment to ensure accessibility for individuals with disabilities. The Department of Justice is considering issuing a supplemental rulemaking proposing to adopt the 2024 USAB standard.

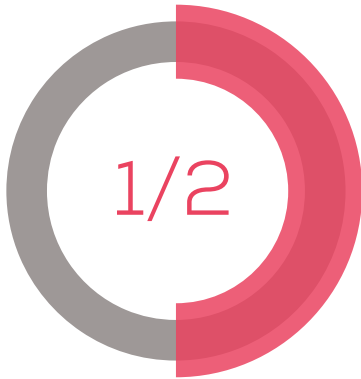

of study respondents indicated it was very important to be compliant with the USAB standard.³

INACCESSIBLE EQUIPMENT IS COSTING YOU


The lack of physical accessibility can adversely affect the quality of care provided, leading to delayed and incomplete care, missed diagnoses, exacerbation of the original disability, and an increased likelihood of the development of secondary conditions.

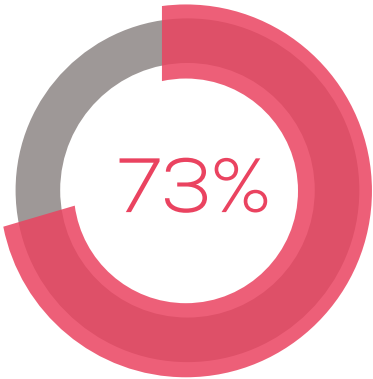

of US adults feel the healthcare system is failing to meet their needs in at least one way.¹



Your patients are changing



By 2030 nearly 1 in 2 adults will have obesity⁴

80 million

In 2020, nearly 60 million Americans were over the age of 65. By 2050, that number is expected to increase to over 80 million⁵

70 million

In 2022, over 70 million Americans reported having a disability⁶

MORE PROCEDURES ARE BEING PERFORMED IN THE OFFICE SETTING

81 million

The number of in-office procedures performed in 2023⁷

44%

In 2023, nearly half of all procedures in the US were performed in the office setting⁷

18%

The estimated increase in the volume of in-office procedures by 2032⁸



SCAN TO LEARN MORE.

The Future of Patient Care is Now

The right procedure room equipment can make a crucial difference in both patient outcomes and caregiver safety. Particularly for patients with mobility limitations, accessible in-office procedure environments are essential. Unfortunately, many procedure chairs on the market today can create barriers to patient access. **Meet the Midmark® 631 Procedure Chair—the first and only US Access Board compliant procedure chair.**



- Midmark 631 Procedure Chair Low Seat Height
- Average Procedure Chair Low Seat Height

Accessible care for **96%** of patients who use wheelchairs.⁹

What makes the 631 compliant?

The Midmark 631 has a US Access Board compliant 17-inch low seat height (while maintaining a 39 inch-high seat height), 28- or 32-inch-wide transfer surface and ample base clearance that is compatible with patient lifts and helps ensure safe patient transfer with no interference. US Access Board compliant Articulating Knee Crutches support the patient's thigh, knee and calf during lower body exam and procedures.



- 01 The compliant Patient Support Rails assist patients in accessing the procedure chair and provide a stable gripping surface while repositioning on the chair.
- 02 The Midmark 631 has a US Access Board compliant 17-inch low seat height (while maintaining a 39-inch high seat height.)
- 03 Transfer patients on the 28- or 32-inch-wide compliant transfer surface.
- 04 The chair is compatible with patient lifts and helps ensure safe patient transfer with no interference.
- 05 US Access Board compliant Articulating Knee Crutches support the patient's thigh, knee and calf during lower body exam and procedures.



SCAN TO SEE A PATIENT TRANSFER.



SCAN TO LEARN MORE.



SCAN TO SEE OUR KNEE CRUTCHES.

Better position caregivers for in-office procedures


No matter the type of procedure, proper positioning is necessary for unobstructed access to the patient and a clear view of the procedure site. Caregiver ergonomics and precise positioning come standard with the Midmark® 631 Procedure Chair. 8-way powered positioning gives you the ability to effortlessly move patients into the most effective positions.

1 out of 5

of all workplace injuries reported in the US is healthcare related.¹⁰

3x

Healthcare workers are almost three times as likely to suffer from work-related injuries than construction workers.¹⁰

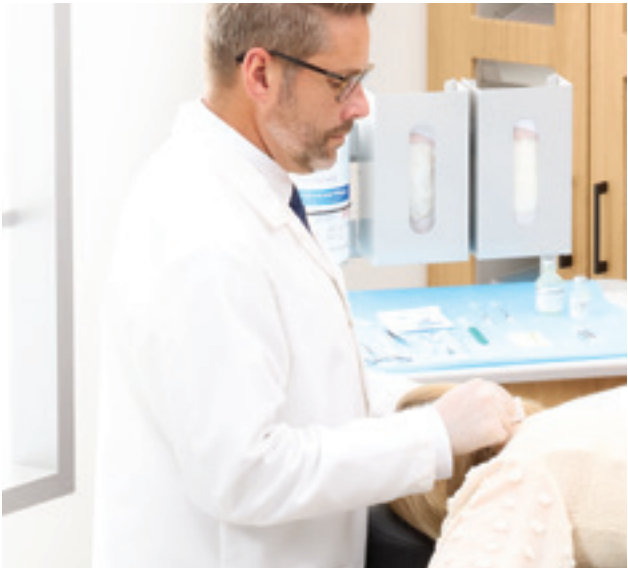

CAREGIVER ERGONOMICS

When performing in-office procedures, it's important to choose a procedure chair that provides clear access to the patient and procedure site. But have you considered caregiver ergonomics?

The Midmark 631 Procedure Chair is designed with features that help ensure ample access to the patient while maintaining a proper working position whether seated or standing.

Precise medical positioning



Lithotomy
Position patients for lower-body procedures



Elevated Flat
Can improve access and visibility to the patient's head, neck and torso



Semi-Fowler
Can improve patient comfort and provide better ergonomics for the caregiver



Trendelenburg
Can be used as a first-line treatment of acute hypotension and shock



Intelligent features to help make time with patients more efficient

As the number of procedures performed in office settings increases and the number of patients you see grows, you're going to want to make the most of the time you have with them. That's why it's good to have a Midmark® 631 Procedure Chair by your side.

STANDARD FEATURES

ACTIVE SENSING TECHNOLOGY®



Avoid impact or disruption while moving the chair. Active sensing technology pauses chair movement when disrupting impact is detected.

MOTION PROFILING®



Allows providers to position patients comfortably on the chair without the need to readjust to maintain head and back support.

FOOT EXTENSION



Extend the chair footrest to accommodate the needs of taller patients.

DUPLEX RECEPTACLES



Hospital-grade, duplex receptacles located on each side of the chair provide power for accessories used during medical procedures.

QUICK CHAIR®



The Quick Chair function (available on the foot control only) saves time by moving the chair into the entry/exit position.

HOME FUNCTION



The chair home function located on the hand and foot controls automatically lowers only the chair base so patients may enter or exit the chair.



LOWER BODY PROCEDURES

Standard features such as a paper roll holder, stirrups and a debris tray provide the precise positioning, support and debris management ideal for lower-body procedures.



SCAN TO LEARN MORE.



Accessories

Adjustable Headrest Design

The standard articulating headrest allows you to tilt the patient’s head or adjust for different procedures, helping improve access and patient comfort. Simply loosen the knob, rotate the headrest up or down and tighten without the use of tools.



STANDARD HEADREST



12.7" H x 12.4" W

OVAL HEADREST



12.7" H x 12.3" W

EXTENDED HEADREST



12.7" H x 12.4" W

U-SHAPED HEADREST



8" H x 11.5" W

RECTANGULAR HEADREST



12" H x 18" W



SCAN TO
LEARN MORE.



ACCESSORIES

PATIENT SUPPORT RAILS



Required for US Access Board Compliance. Provide patients with a 1¼ inch diameter continuous gripping surface for entering, exiting or repositioning on the procedure chair.

PATIENT SUPPORT RAILS +



Required for US Access Board Compliance. Help achieve proper positioning of the patient's arm for phlebotomy procedures and blood pressure capture.

ARTICULATING KNEE CRUTCHES



Required for US Access Board Compliance. Enhance patient leg support and comfort during lower body exam and procedures

CHAIR ARMS



Fits 28" and 32" upholstery widths

SEAT RAILS



Surgical size 1 1/8"

BACK + BASE ACCESSORY RAILS



Surgical size 1 1/8" and standard size 1"

HAND SURGERY ARMBOARD



8.5" W x 26" L

SECURITY STRAPS



Adjustable width and location

RITTER® 253 LED LIGHT



Available in chair mount (spline or rail), wall mount and mobile options

ARTICULATING ARMBOARD



7" W x 24" L

VISION BLOCK SCREEN



Blocks patient's line of sight



SCAN TO
LEARN MORE.




COLOR OPTIONS

STANDARD UPHOLSTERY COLORS

	Mist 813
	Stone 814
	Restful Path 858
	Iron Ore 851
	Lunar Gray 845
	Obsidian 857
	Oasis 843
	Soothing Blue 855
	Dream 847
	Mineral 844
	Healing Waters 848
	Shaded Garden 853
	Citrus 849
	Sandy Retreat 850
	Curative Copper 846
	Cranberry 859
	Dark Linen 856
	Latte 860
	Robust Brown 852
	Deep Earth 854

ULTRAFREE UPHOLSTERY COLORS

	UltraFree Stone 865
	UltraFree Restful Path 868
	UltraFree Obsidian 867
	UltraFree Harbor 861
	UltraFree Wheatgrass 862
	UltraFree Spice 863
	UltraFree Cranberry 869
	UltraFree Dark Linen 866
	UltraFree Latte 870
	UltraFree Branch 864

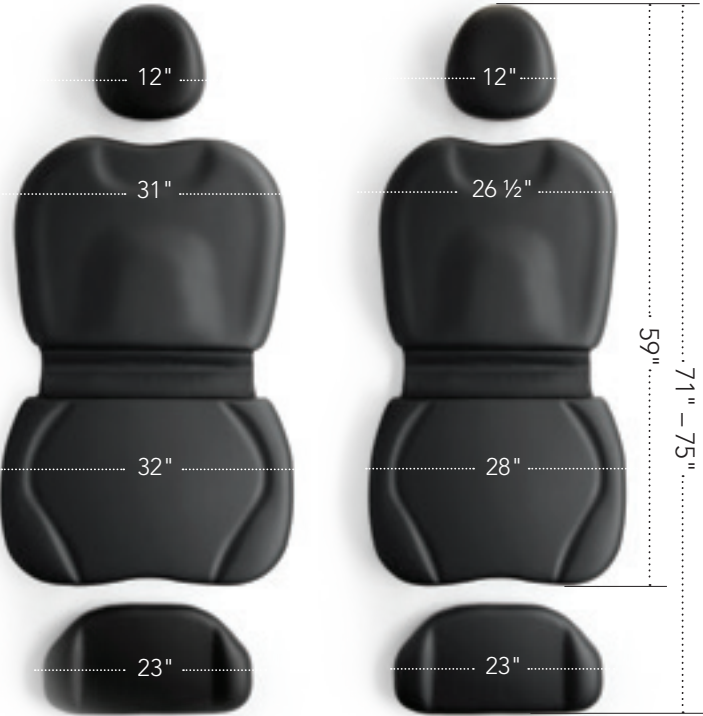

UPHOLSTERY

Available in 28" and 32" widths to accommodate a range of patient sizes.

SERVICES + SUPPORT

TECHNICAL SPECIFICATIONS

View technical specifications for the Midmark® 631 Procedure Chair.



SCAN TO
VIEW SPECS.

REPAIR + SERVICE

Explore available support and service plans so you can obtain the level of coverage you need to keep your medical equipment and devices operational. This includes periodic maintenance and periodic inspection plans, as well as extended warranty plans.



SCAN FOR
SUPPORT.

MIDMARK LIVE DESIGN

Our in-house design experts are ready to help you every step of the way.



SCAN TO
VIEW VIDEO.

PROTECT YOUR INVESTMENT

Register your warranty today to receive prompt support when you need it.



SCAN TO VIEW.

MIDMARK DELIVERY SERVICES

Coordination, delivery and setup right on time, every time.



SCAN TO
VIEW YOUR
OPTIONS.

SOURCES

- <https://www.aapa.org/download/113510/?tmstv=1684243687>
- <https://www.federalregister.gov/documents/2024/07/25/2024-16266/standards-for-accessible-medical-diagnostic-equipment>
- Internal Midmark Conducted Research
- <https://pubmed.ncbi.nlm.nih.gov/31851800/>
- <https://www.census.gov/library/stories/2019/12/by-2030-all-baby-boomers-will-be-age-65-or-older.html>
- <https://www.cdc.gov/media/releases/2024/s0716-Adult-disability.html#:~:text=The%20latest%20data%2C%20from%20the,having%20a%20disability%20in%202022.>
- Retrieved November 2024 from: <https://clarivate.com/coronavirus-resources/?lid=d>
See "Impact on Medical Procedure... tab"
- <https://vizientinc-delivery.sitecorecontenthub.cloud/api/public/content/adad7d916064411aa36f15c901541888?v=1466587d>
- <https://www.access-board.gov/research/human/wheelchair-seat-height/>
- <https://www.bls.gov/charts/injuries-and-illnesses/number-and-rate-of-nonfatal-work-injuries-by-industry.htm>



Designing better care.®



CARB 93120.2 Phase 2 Compliant and TSCA Title VI Compliant

The color examples shown are the best representation of the original material. Actual color may vary slightly. We strongly recommend that you contact Midmark Customer Experience at 1.800.MIDMARK to request a sample before placing your order.

Midmark is an ISO 13485 and ISO 9001 Certified Company. Certain products are not included. See the complete list at: midmark.com/ISO

For more information, contact your authorized Midmark distributor or call: 1.800.MIDMARK

Outside the USA call: 1.937.526.3662 or visit our website: midmark.com

USGBC® and the related logo are trademarks owned by the U.S. Green Building Council® and are used with permission.

© 2025 Midmark Corporation, Versailles, Ohio USA
Products subject to improvement changes without notice.

007-10510-00 Rev. B1 (5/25)

