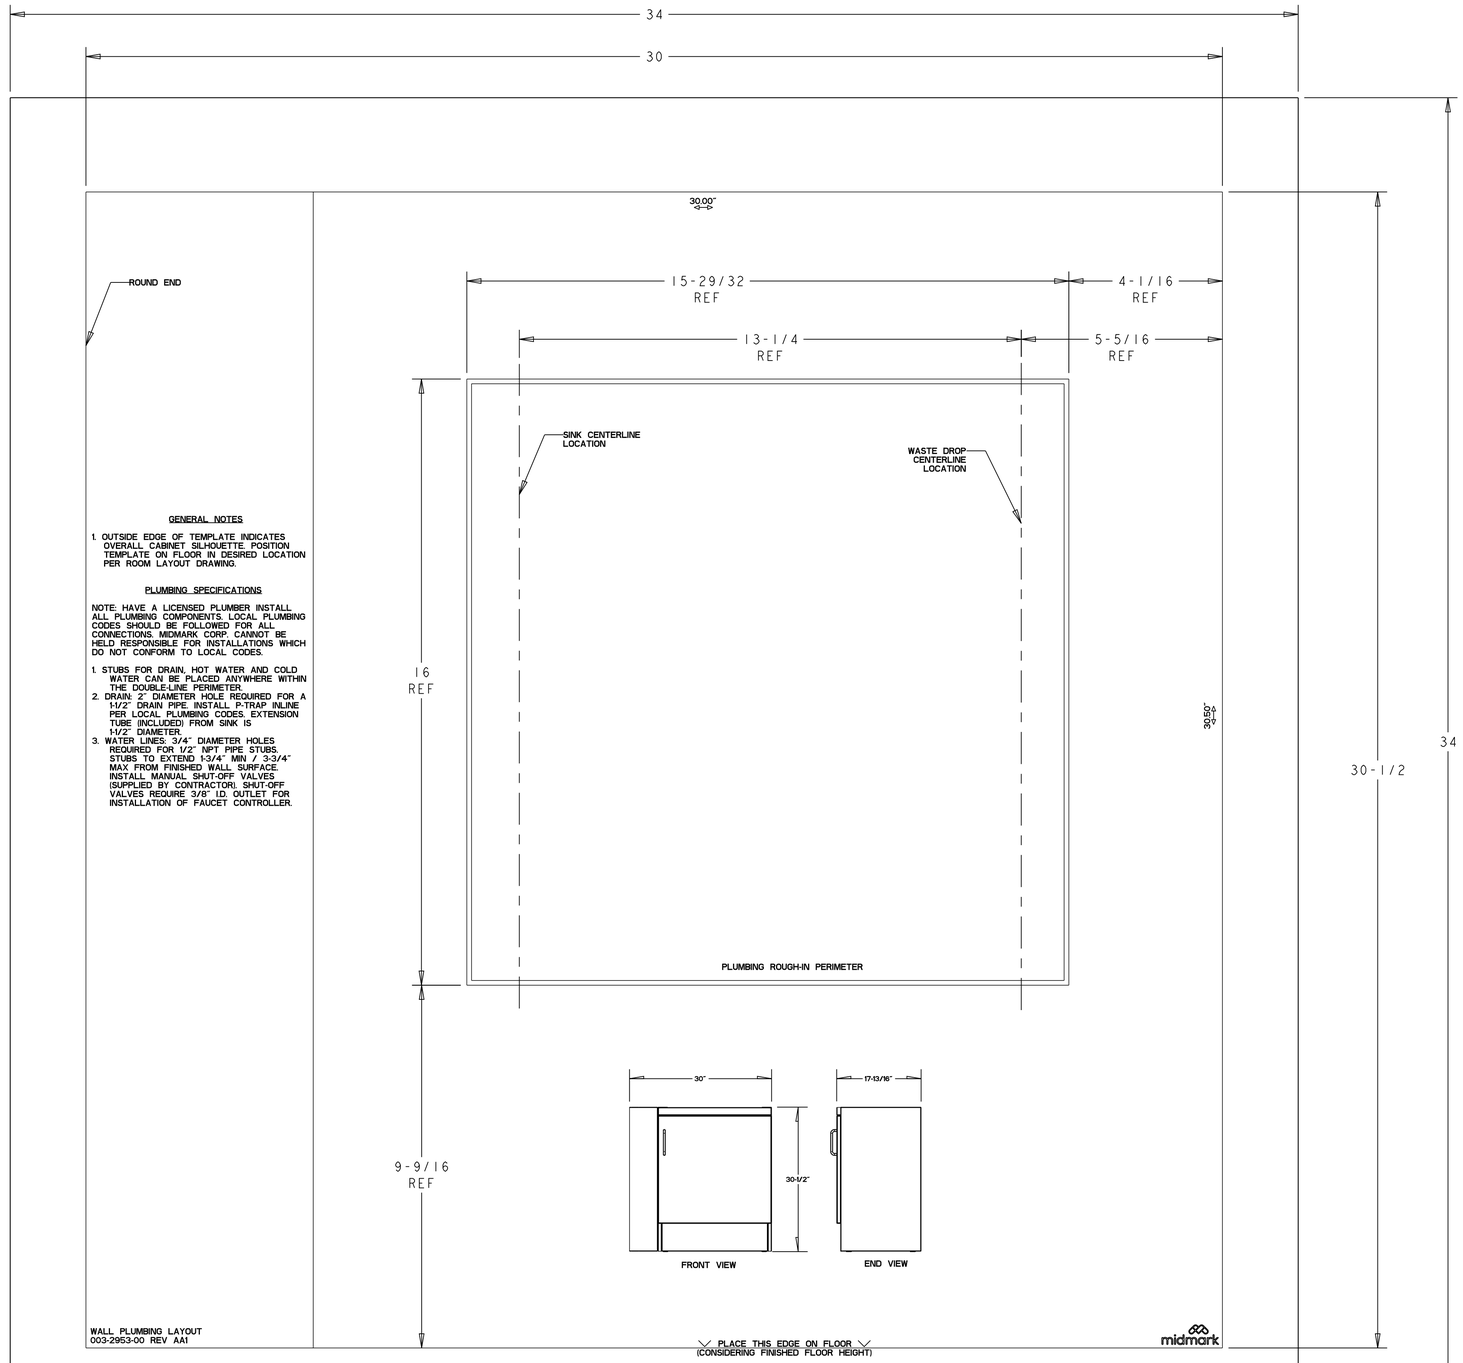

GENERAL NOTES

1. OUTSIDE EDGE OF TEMPLATE INDICATES OVERALL CABINET SILHOUETTE. POSITION TEMPLATE ON FLOOR IN DESIRED LOCATION PER ROOM LAYOUT DRAWING.

PLUMBING SPECIFICATIONS

NOTE: HAVE A LICENSED PLUMBER INSTALL ALL PLUMBING COMPONENTS. LOCAL PLUMBING CODES SHOULD BE FOLLOWED FOR ALL CONNECTIONS. MIDMARK CORP. CANNOT BE HELD RESPONSIBLE FOR INSTALLATIONS WHICH DO NOT CONFORM TO LOCAL CODES.

1. STUBS FOR DRAIN, HOT WATER AND COLD WATER CAN BE PLACED ANYWHERE WITHIN THE DOUBLE-LINE PERIMETER.
2. DRAIN: 2" DIAMETER HOLE REQUIRED FOR A 1-1/2" DRAIN PIPE. INSTALL P-TRAP INLINE PER LOCAL PLUMBING CODES. EXTENSION TUBE (INCLUDED) FROM SINK IS 1-1/2" DIAMETER.
3. WATER LINES: 3/4" DIAMETER HOLES REQUIRED FOR 1/2" NPT PIPE STUBS. STUBS TO EXTEND 1-3/4" MIN / 3-3/4" MAX FROM FINISHED WALL SURFACE. INSTALL MANUAL SHUT-OFF VALVES (SUPPLIED BY CONTRACTOR). SHUT-OFF VALVES REQUIRE 3/8" I.D. OUTLET FOR INSTALLATION OF FAUCET CONTROLLER.

NOTES:
1. MATERIAL: 20# WHITE OFFSET PAPER.
2. INK COLOR: BLACK

ECO NO	DATE	CH BY	CHANGE	REV
.	.	.	.	.
.	.	.	.	.
ECO063469	9/18/18	PTR	ADDED DIMENSIONS AND UPDATED LOGO.	AA1
C2729	4/27/16	BLS	RELEASED	A1

THIS PRINT AND THE INFORMATION CONTAINED THEREIN ARE PROPERTY OF MIDMARK CORPORATION ARE FURNISHED TO THE HOLDER IN CONFIDENCE AND ARE NOT TO BE REPRODUCED,USED,OR DISCLOSED TO OTHERS WITHOUT THE EXPRESS WRITTEN PERMISSION OF MIDMARK CORPORATION

INCH [MILLIMETER] INCH [MILLIMETER]

UNSPECIFIED GENERAL TOLERANCES

ANGULAR +/- 2.0°
FRACTIONAL +/- 1/4
DECIMAL .XX +/- 0.03
DECIMAL .XXX +/- 0.015

COMMERCIAL TOLERANCES SHALL APPLY ON BAR, ROD, WIRE, SHEET, ETC.

ITEM	QTY	PART NUMBER	DESCRIPTION

MATERIAL SPEC
.
.

midmark

SCALE 0.500 | CK BY DATE

SHEET 1 OF 2

PREPARED BY BSTACHLER | DATE 04/27/16

PART NAME TEMPLATE, 30R LH WALL

APPROVED BY | DATE

PART NUMBER 003-2953-00 | REV AA1

PRATHGE 9/25/2018 7:31:50 AM

File is formatted to print at (36in. x 36in.) To request printed template, contact Midmark Corporation at 1-800-643-6275.

ROUND END

GENERAL NOTES

1. OUTSIDE EDGE OF TEMPLATE INDICATES OVERALL CABINET SILHOUETTE. POSITION TEMPLATE ON FLOOR IN DESIRED LOCATION PER ROOM LAYOUT DRAWING.

PLUMBING SPECIFICATIONS

NOTE: HAVE A LICENSED PLUMBER INSTALL ALL PLUMBING COMPONENTS. LOCAL PLUMBING CODES SHOULD BE FOLLOWED FOR ALL CONNECTIONS. MIDMARK CORP. CANNOT BE HELD RESPONSIBLE FOR INSTALLATIONS WHICH DO NOT CONFORM TO LOCAL CODES.

1. STUBS FOR DRAIN, HOT WATER AND COLD WATER CAN BE PLACED ANYWHERE WITHIN THE DOUBLE-LINE PERIMETER.
2. DRAIN: 2" DIAMETER HOLE REQUIRED FOR A 1-1/2" DRAIN PIPE. INSTALL P-TRAP INLINE PER LOCAL PLUMBING CODES. EXTENSION TUBE (INCLUDED) FROM SINK IS 1-1/2" DIAMETER.
3. WATER LINES: 3/4" DIAMETER HOLES REQUIRED FOR 1/2" NPT PIPE STUBS. STUBS TO EXTEND 1-3/4" MIN / 3-3/4" MAX FROM FINISHED WALL SURFACE. INSTALL MANUAL SHUT-OFF VALVES (SUPPLIED BY CONTRACTOR). SHUT-OFF VALVES REQUIRE 3/8" I.D. OUTLET FOR INSTALLATION OF FAUCET CONTROLLER.

30.00"

SINK CENTERLINE LOCATION

WASTE DROP CENTERLINE LOCATION

30.50"

PLUMBING ROUGH-IN PERIMETER

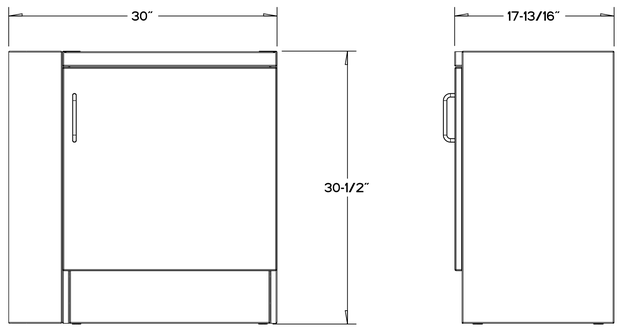

FRONT VIEW

END VIEW

WALL PLUMBING LAYOUT
003-2953-00 REV AA1

PLACE THIS EDGE ON FLOOR
(CONSIDERING FINISHED FLOOR HEIGHT)

midmark

PRATHGE 9/25/2018 7:31:50 AM